



CMR 363, 10 hPa F.S., 8 VCR






Similar Image

CMR 363, 10 hPa F.S., 8 VCR

- Precise pressure measurement independent of type of gas
- Measurement range up to four decades
- Gauge for connection to TPG
- Flange size: DN 8 VCR
- Measurement range from $1 \cdot 10^{-3}$ hPa to 11 hPa
- Minimal zero drift
- Sensor in ceramic technology
- No memory effects
- Materials employed have identical temperature coefficients
- Precise temperature compensation
- Calibration test report included in delivery

Dimensions

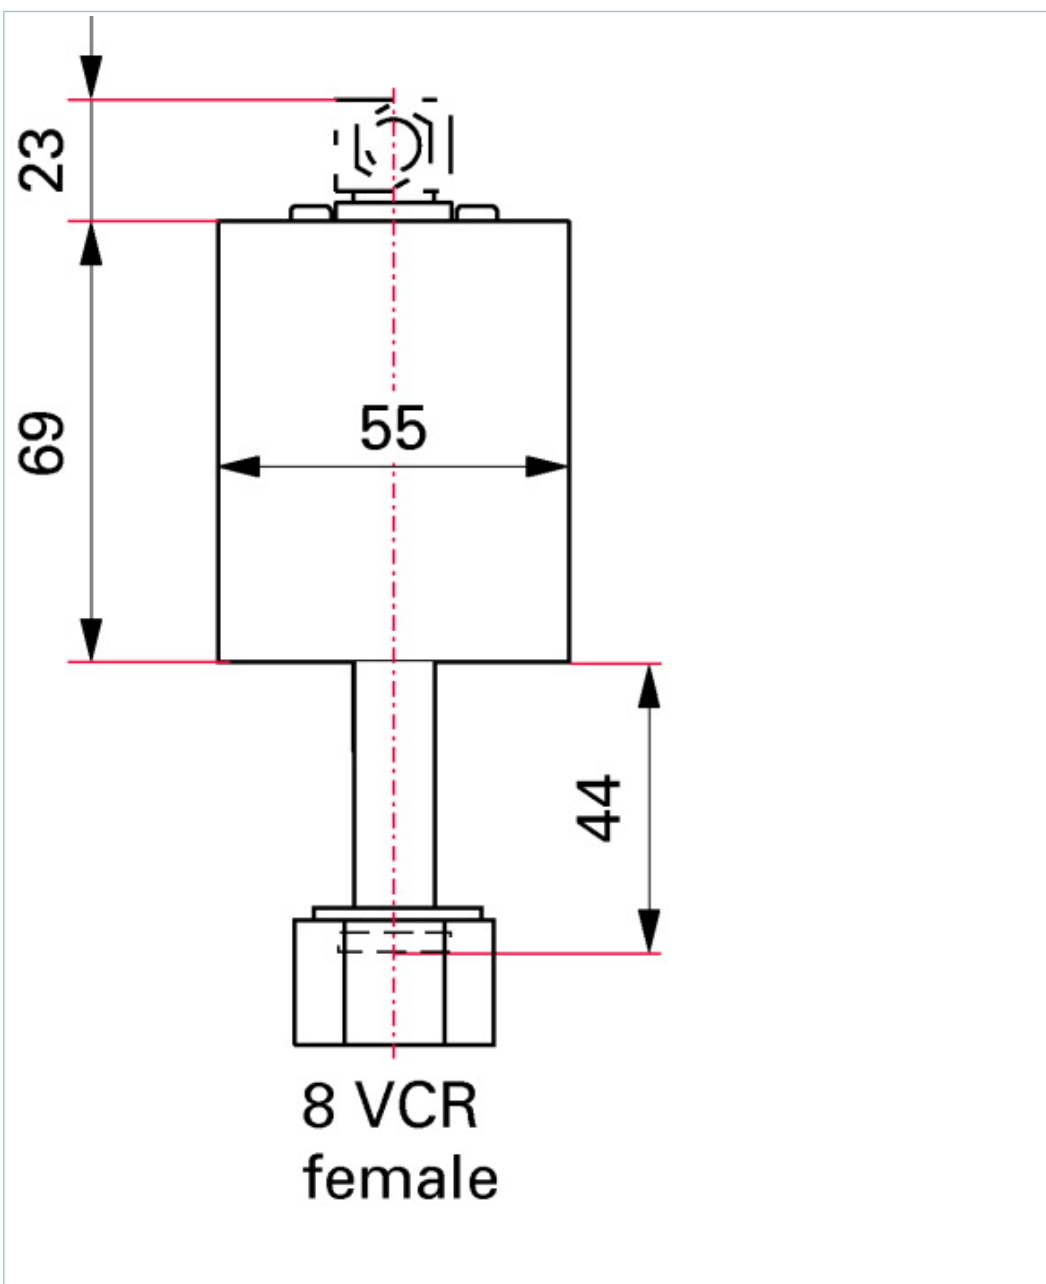

Technical Data	CMR 363, 10 hPa F.S., 8 VCR
Accuracy	0.20 % of reading
Bakeout temperature max. at the flange	$\leq 110\text{ }^{\circ}\text{C}$ $\leq 230\text{ }^{\circ}\text{F}$ $\leq 383\text{ K}$
Full Scale	10 hPa 7.5 Torr 10 mbar
Measurement range max.	11 hPa 8.25 Torr 11 mbar
Measurement range min.	$1 \cdot 10^{-3}\text{ hPa}$ $7.5 \cdot 10^{-4}\text{ Torr}$ $1 \cdot 10^{-3}\text{ mbar}$
Membrane and measuring chamber	Ceramics (Al_2O_3 99.5 %)
Method of measurement	Capacitance
Nominal diameter	Cajon 8 VCR
Output signal: Minimum load	10 k Ω
Output signal: Pressure range	1 - 9.8 V
Output signal: Sensor error above	> 9.8 V
Output signal: Sensor error below	< 0.4 V
Pipe and flange	Stainless steel
Pressure max.	2,000 hPa 1,500 Torr 2,000 mbar
Protection category	IP30
Resolution	0.003 % F.S.
Sensor cable length	$\leq 120\text{ m}$
Supply: Power consumption max.	$\leq 1\text{ W}$
Supply: Voltage	14-30 V DC
Temperature: Operating	$5\text{-}50\text{ }^{\circ}\text{C}$ $41\text{-}122\text{ }^{\circ}\text{F}$ $278\text{-}323\text{ K}$
Temperature: Storage	$-40\text{-}65\text{ }^{\circ}\text{C}$ $-40\text{-}149\text{ }^{\circ}\text{F}$ $233\text{-}338\text{ K}$
Temperature effect: on span	0.01 % of reading/ $^{\circ}\text{C}$
Temperature effect: on zero	0.005 % F.S./ $^{\circ}\text{C}$
Volume	$\leq 3.6\text{ cm}^3$
Weight	$\leq 370\text{ g}$

Order number	
CMR 363	PT R24 623

Accessories	
Accessory for ActiveLine gauges and controllers	
Mating connector	B 4707 283 MA
Sensor cable, 3 m	PT 448 250 -T